# Alexis® O

## WOUND PROTECTOR/RETRACTOR*

## Setup Guide



Prepare the surgical site according to standard procedure, making sure the skin is clean and dry.

**1.** Make an incision along the marked incision line.

**2.** Insert the Alexis O wound protector's green ring into the operative site.

**3.** Carefully check to ensure that no bowel or tissue entrapment has occurred before retraction is initiated.




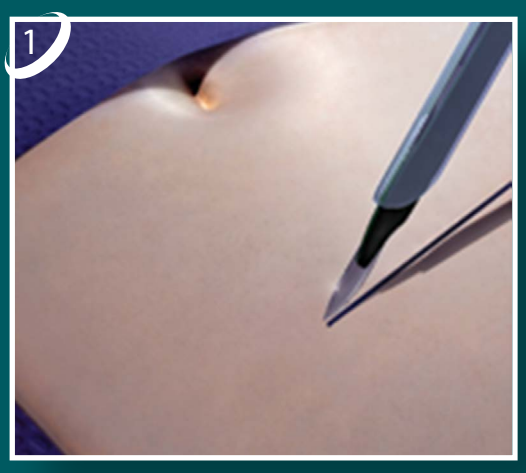


**4.** Gently grasp the white retraction ring at 10 and 2 o'clock and pull up until the green ring sits tightly against the peritoneal layer. Roll inward until desired retraction is achieved.

**5.** Double check to ensure that no bowel or tissue entrapment has occurred. (See figure 3)

**6.** Perform procedure through 360° retracted and protected incision site.

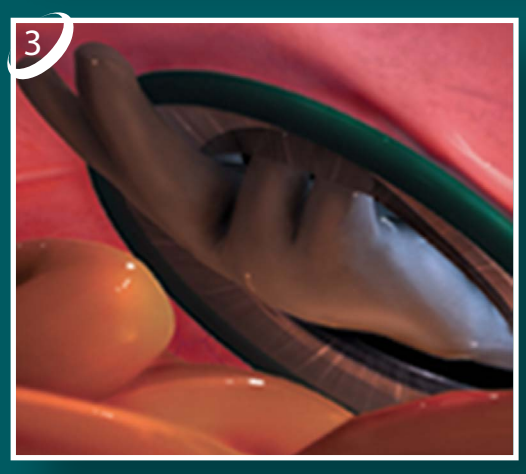


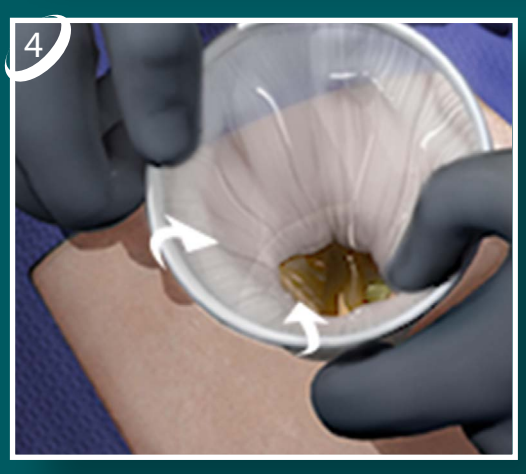**7.** Retrieve the Alexis O protector by simply removing the green inner ring from the peritoneal cavity.

*Refer to complete instructions for use.

**http://contact.appliedmedical.com/**

For more information
**www.appliedmedical.com/alexis**

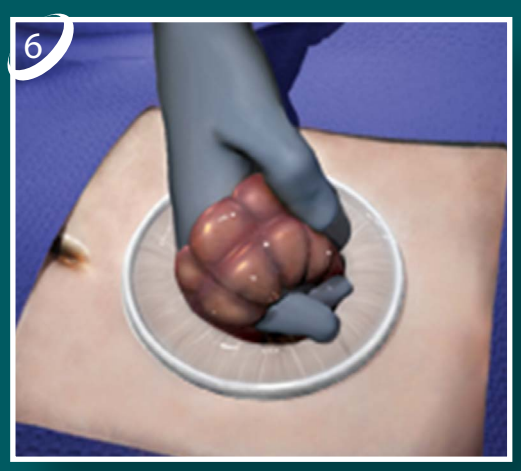Applied Medical

© 2016 Applied Medical Resources Corporation. All rights reserved. Applied Medical, the Applied Medical logo design, ProTerra, the ProTerra logo designand marks designated with a ® are trademarks of Applied Medical Resources Corporation, registered in one or more of the following countries: Australia, Canada, Japan, the United States and/or the European Union. SC01424J